


## SETTING THE DATE AND TIME

Press the On/Off button to turn the meter on. To enter Set-up mode, hold On/Off button for 2 seconds. Press the Up/Down button to reach desired setting. Press On/Off button move to next set up mode.



To exit set-up mode, hold the On/Off button for 2 seconds.

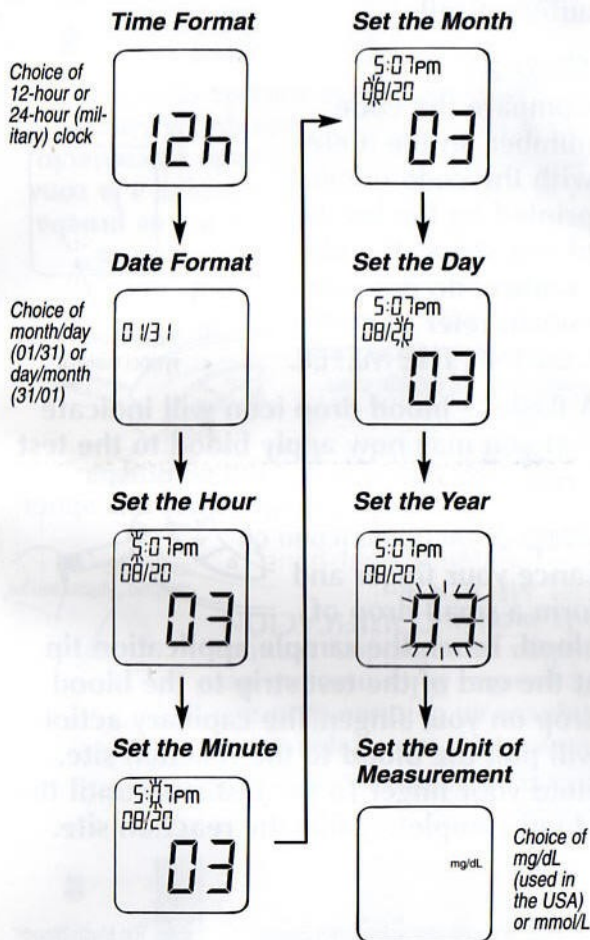

Minneapolis, MN 55439 USA  
Phone: 800-566-8558  
Fax: 952-646-3110  
www.hypoguard.com


P/N 1517-01  
Rev 1/04

## PERFORMING A CONTROL SOLUTION TEST

Before performing a control solution test, always check the expiration date (Exp.) of the control solution. Always use within 90 days of first opening. Replace the cap immediately after each use.

### Step 1



Insert the top of the test strip into the test strip port of the meter (as shown). The meter turns on automatically.




### Step 2

Confirm that the code number on the display matches the code number on the bottle of test strips. If not, refer to CODING THE METER.


### Step 3 IMPORTANT

Press the Up or Down button to display the  in the upper right-hand corner of the display screen. If you do not display the  the control solution result will not be valid.



### Step 4

Apply a drop of control solution to the sample application tip when  flashes.



### Step 5


Verify that the result is within the range printed on the test strip bottle you are using. If the result falls within the range on the bottle, the meter is working correctly.



# Micro-draw™

Blood Glucose Monitoring System

# Advance

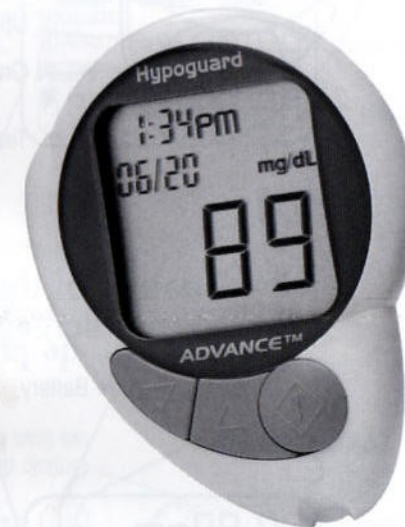


## Quick Start Guide

For additional assistance call  
Customer Service at  
1-800-566-8558

Test Strip Port

## Explanation of the full display screen

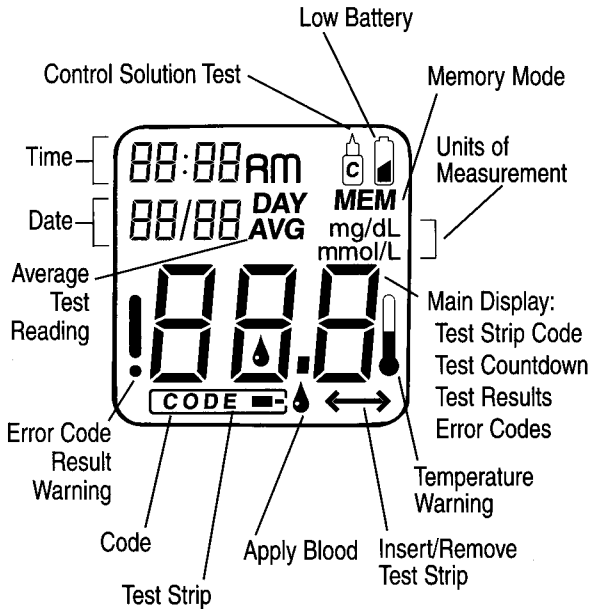

the code chip into the port on the side of the meter as shown.



### Step 2

Insert the top of the test strip into the meter test strip port.

The meter will turn on automatically. The screen briefly displays all symbols, then displays the code number.

### Step 3

Verify the code number displayed on the screen matches the code number on the bottle of test strips you are using. If the codes match, begin testing.

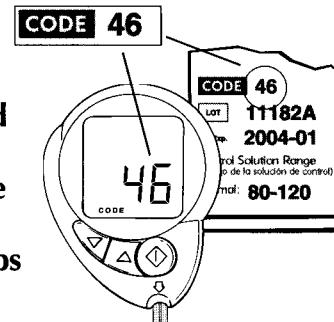


of test strips. If code numbers do not match, refer to CODING THE METER.

A flashing blood drop icon that you may now apply blood strip.

### Step 3

Lance your finger and form a small drop of blood. Touch the sample application site at the end of the test strip to the drop on your finger. The capillary action will pull the blood to the reaction site. Hold your finger to the test strip until the blood completely fills the reaction site.



If the reaction site is not completely filled, you may get inaccurate results.

The meter counts down and displays the result.